

DETECTION OF BIOLOGICAL AEROSOLS BY MALDI ON-LINE AEROSOL TOF MS

Ben L.M. van Baar,¹ Michael A. Stowers,² Arjan L. van Wuijckhuijse,² Charles E. Kientz,¹ Brian Scarlett,² Jan C.M. Marijnissen,² and Ruud W. Busker¹

1. TNO Prins Maurits Laboratory, P.O. Box 45, NL-2280 AA Rijswijk (ZH), The Netherlands.
2. Delft University of Technology, Faculty of Applied Sciences, Julianalaan 136, NL-2628 BL, Delft, The Netherlands.

ABSTRACT

Matrix-assisted laser desorption/ionisation (MALDI) mass spectra were obtained from single biological aerosol particles using an aerosol time-of-flight mass spectrometer (ATOFMS). The inlet to the ATOFMS was coupled with an evaporation/condensation flow cell that allowed the aerosol to be coated with matrix material as the sampled stream entered the spectrometer. Mass spectra were generated from aerosols of gramicidin-S, erythromycin, insulin and cytochrome c, or of *Bacillus subtilis* var niger spores. The results give a proof of principle that MALDI ATOFMS can provide nearly real-time identification of biological aerosols.

INTRODUCTION

Single particle aerosol mass spectrometry has developed since the late 1980s.¹ A system for aerosol mass spectrometry, was originally constructed at the Delft University of Technology.² This system, the ATOFMS, consists of a particle-beam like aerosol inlet, a HeNe laser for particle sizing and ionization triggering, an UV ionization laser and a time-of-flight mass analyzer. This system was recently further modified to achieve bio-aerosol detection, with the ultimate goal of establishing a generic bio-aerosol alarm.

RESULTS

First, a device was constructed for the on-line coating of aerosol particles with a matrix compound. This allowed more efficient ionization, through on-line aerosol MALDI MS.³ Low mass peptides, erythromycin (~700 Da) and gramicidin S (~1,040 Da) and glycan type material from *Bacillus subtilis* var niger spores (~1,230 Da) was observed in typical MALDI-ATOFMS mass spectra.

Next, the upper mass range limit of 2000 Da was extended by instrument modifications to the mass spectrometer. With the extended mass range and matrix addition, spectra of larger peptides were obtained; in Figure 1, an example is shown of a spectrum obtained from cytochrome c aerosol.

Report Documentation Page

Form Approved
OMB No. 0704-0188

Public reporting burden for the collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to a penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number.

1. REPORT DATE 00 JAN 2002	2. REPORT TYPE N/A	3. DATES COVERED -			
4. TITLE AND SUBTITLE Detection Of Biological Aerosols By Maldi On-Line Aerosol Tof Ms		5a. CONTRACT NUMBER			
		5b. GRANT NUMBER			
		5c. PROGRAM ELEMENT NUMBER			
6. AUTHOR(S)		5d. PROJECT NUMBER			
		5e. TASK NUMBER			
		5f. WORK UNIT NUMBER			
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) TNO Prins Maurits Laboratory, P.O. Box 45, NL-2280 AA Rijswijk (ZH), The Netherlands; Delft University of Technology, Faculty of Applied Sciences, Julianalaan 136, NL-2628 BL, Delft, The Netherlands		8. PERFORMING ORGANIZATION REPORT NUMBER			
		10. SPONSOR/MONITOR'S ACRONYM(S)			
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)		11. SPONSOR/MONITOR'S REPORT NUMBER(S)			
		12. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release, distribution unlimited			
13. SUPPLEMENTARY NOTES This article is from ADA409494 Proceedings of the 2001 ECBC Scientific Conference on Chemical and Biological Defense Research, 6-8 March , Marriott's Hunt Valley Inn, Hunt Valley, MD.					
14. ABSTRACT					
15. SUBJECT TERMS					
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT UU	18. NUMBER OF PAGES 2	19a. NAME OF RESPONSIBLE PERSON
a. REPORT unclassified	b. ABSTRACT unclassified	c. THIS PAGE unclassified			

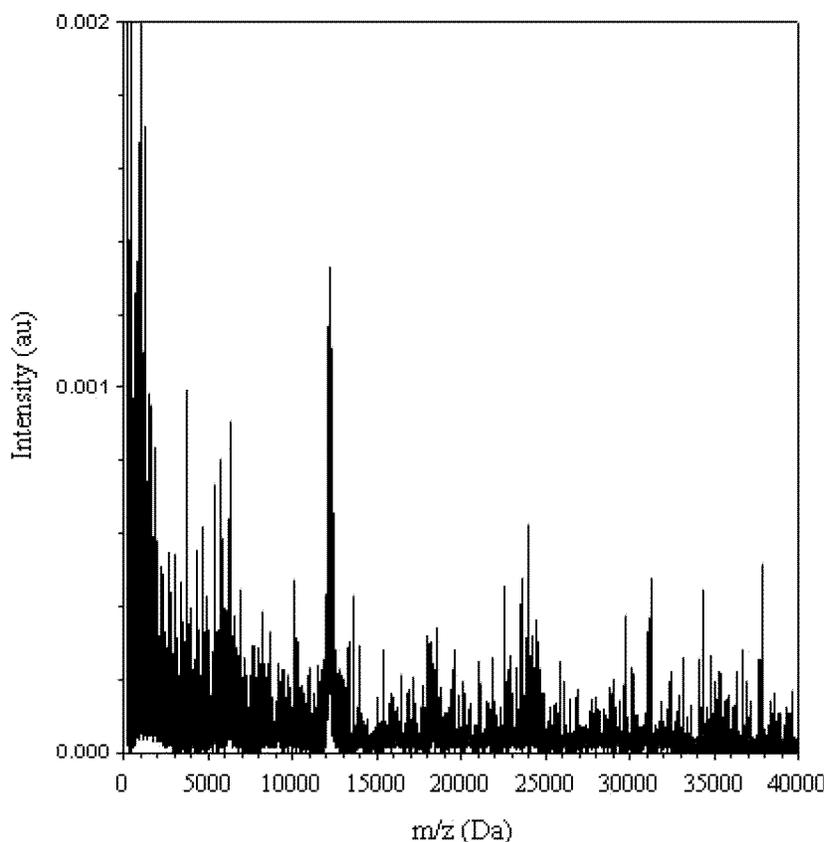


Figure 1. MALDI-ATOFMS spectrum obtained from an aerosol of cytochrome c (MW_{av} 12,270 Da), premixed with ferulic acid matrix.

Most biomarker signals from bacteria, as observed in common MALDI MS, fall in the mass range up to 30,000. Therefore, observations of proteins in this range, with the MALDI-ATOFMS, is a proof of principle that bacteria fingerprints can be obtained in real-time (seconds).

Currently, the MALDI-ATOFMS system is being modified for selective ionization of bio-aerosol particles, by on-the-flight distinction of biological particles from common organic and inorganic particles. This selective ionization will be used to increase the detection efficiency for bio-aerosol particles.

ACKNOWLEDGMENT

The authors thank The Netherlands Ministry of Defence for continued support to the project (under number 98A420).

REFERENCES

- ¹ D.T Suess and K.A Prather, Chem. Rev. **99** (1999), 3007-3035.
- ² O. Kievit, M. Weiss, P.J.T. Verheijen, J.C.M. Marijnissen, B. Scarlett, Chem. Eng. Commun. **151** (1996), 79-100; and M. Weiss, P. Verheijen, J.C.M. Marijnissen, B. Scarlett, J. Aerosol Sci. **28** (1997), 159-171.
- ³ M.A. Stowers, A.L. van Wuijckhuijse, J.C.M. Marijnissen, B. Scarlett, B.L.M. van Baar, C.E. Kientz, Rapid Commun. Mass Spectrom. **14** (2000), 829-833.